
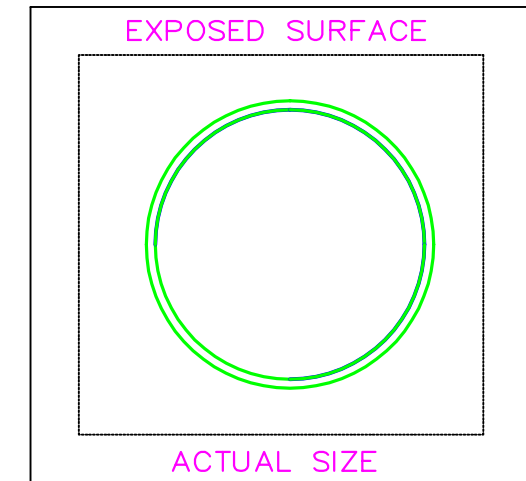


SECTION NO.

950-103

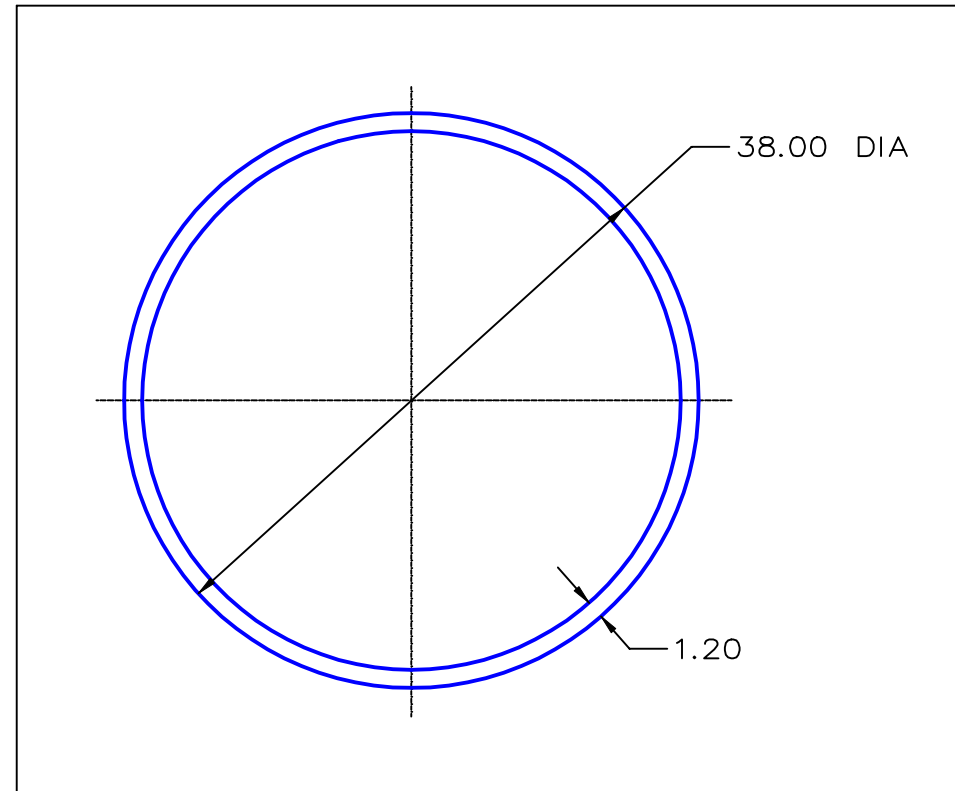

SECTION DATA:

$I_{xx} = 23\,510 \text{ mm}^4$
 $I_{yy} = 23\,510 \text{ mm}^4$
 $\text{Theta} = 0.$
 $\text{RadG}_x = 13. \text{ mm}$
 $\text{RadG}_y = 13. \text{ mm}$
 $X_{\text{Left}} = 19.0 \text{ mm}$
 $X_{\text{Right}} = 19.0 \text{ mm}$
 $Y_{\text{Top}} = 19.0 \text{ mm}$
 $Y_{\text{Bot}} = 19.0 \text{ mm}$
 $Z_{xx\text{top}} = 1\,237 \text{ mm}^3$
 $Z_{xx\text{bot}} = 1\,237 \text{ mm}^3$
 $Z_{yy\text{left}} = 1\,237 \text{ mm}^3$
 $Z_{yy\text{right}} = 1\,237 \text{ mm}^3$

1.2 TYP WALL THICKNESS
UNLESS OTHERWISE SPECIFIED

0.40 RADIUS ON ALL OUTSIDE CORNERS
UNLESS OTHERWISE SPECIFIED

EXTRUDED FINISH : ARCHITECTURAL

			A	AREA 138.7 SQ MM WEIGHT 0.376 KG M PERIMETER 231.2 MM ANOD PERIM 119.4 MM PAINT PERIM 119.4 MM C CIRCLE DIA 38. MM FACTOR 615. ALLOY 6063 TEMPER T6	 A.C.N 010 828 234 1082 KINGSFORD SMITH DRIVE, EAGLE FARM, QUEENSLAND, 4009 PO BOX 1376, EAGLE FARM BC, 4009 PHONE : (07) 3877 2833 FAX : (07) 3877 2890	CUSTOMER		G.JAMES EXTRUSION Co.	
						CUSTOMER PART NAME NO.		38 x 1.2 ROUND TUBE	
					SCALE		TOLERANCES IN ACCORDANCE WITH AS 1866-1986 APPLY UNLESS OTHERWISE SPECIFIED		
					2:1				
NO	DATE	DR	REVISION			DRAWN	CHECK	DATE	DWG. NO.
						PS		14/01/92	950-103